

## STABILITY EVOLUTION OF ALFA GATE BIOACTIVE COATING® IMPLANTS DURING HEALING PERIOD

### Summary

Commercial oral implantology grew during the 1980s. Osseointegration was being used to permanently affix bridges and individual teeth into patients' mouths. The implants proved to be successful in over 90% of the cases. The modern dental implant had arrived!

Over the next two decades, technology has only continued to improve the process. For instance, slight modifications to the titanium proved to increase healing time. As time goes by and as the practice of dentistry advances, patients will continue to see dental implants becoming quicker, easier, and less painful.

Key words: dental implant, implant stability quotient (ISQ), implant surface modification, osseointegration, Alfa Gate dental implants.

### Introduction:

Placement of dental implants in edentulous people is an efficacious method for the replacement of missing teeth [13]. According to the literature, more than 1300 types of dental implants are available, in different materials, shapes, sizes, lengths and with different surface characteristics or coatings [6]. The success rate for osseointegration of dental implants has been shown to be very high for many different designs and brands of implants [23, 11,18]. Primary stability, which is one of the most important criteria of implant integration and success rate, depends on especially of the geometry of the implants (length, diameter, shape, and thread) besides the surgical technique, volume, and mechanical quality of local bone [42,21]. During the

Mohamad Zahalka,  
Valentin Topalo,  
*prof. univ.*

osseointegration healing period, bone gradually forms inside the implant threads and thus, the secondary stability is attained by an incremental degree of bone to implant contact [37]. It is proportioned with implant success rate, depends of bone remodelling induced by a mechanical stress situation during the initial phase of bone healing and surface modification of the implants [12]. According to current literature, there are discussions concerning ability of implants to withstand early or immediate loading in order to reduce waiting time for the patient. In addition to mentioned parameters of the primary and secondary stability, the implant surface osteologic characteristics are factors which affect the implant bone response and quality of the bone implant interface [4,29]. Surface treatment helps to enhance secondary stability after insertion by promoting osseointegration [25,12,16]. Various methods have been developed and tested in order to coat metal implants, e.g. plasma-spraying, sputter-deposition, sol-gel coating, electrophoretic deposition or biomimetic precipitation [29,2]. Recently a new surface implant system with a completely resorbable, fixed adhesive calcium-phosphate (CaP) coating (Bioactive®) is available (figure 1). It is a 5 grade titanium alloy with microstructure, internal hexagon, spiral, conical, self drilling, self tapping, double thread system, with deep and especially sharp threads decreasing towards the implant shoulder, enabling implant self-retention. Bioactive® coating is a newly developed electrochemical process for implant coating in an aqueous solution containing calcium and phosphate ions. According to the manufacture dates the calcium phosphate coating properties are: large active surface with high capillarity effect on blood; stimulation of the body's own osteosynthesis; substitution of Bioactive® coating by young bone directly on the implant surface within 6 – 10 weeks post-operative; low coating thickness of 20-30 µm.

Therefore, the aim of the present study was to investigate the early outcome of a recently developed dental implant with CaP coating (Alfa Gate) in 6 weeks of usage in mandibular clinical situations.

#### **Purpose and tasks**

1- To investigate the early outcome of a dental implant with bioactive Calcium-phosphate (CaP) coating in the first 6 week of usage in mandibular clinical situations, for determination if it is possible early prosthetic loading.

1- Methodical elaboration for measurements of implant stability dynamics.

1- Determination of critical time in implant dynamics.

#### **Different times for loading dental implants**

Primary implant stability and lack of micromovements are considered to be two of the main factors necessary for achieving predictable high success of osseointegrated oral implants (Albrektsson 1981). A successful osseointegrated oral implant is anchored directly to bone, however, in the presence of movement a soft tissue interface may encapsulate the implant (Brunski 1979) causing its failure. To minimize the risk of soft tissue encapsulation, it has been rec-

ommended to keep the implants load-free during the healing period (3 to 4 months in mandibles and 6 to 8 months in upper jaws) (Branemark 1977).

In general, during the healing period removable prostheses are used, however many patients find these temporary prostheses rather uncomfortable and it would therefore be beneficial if the healing period could be shortened without jeopardizing implant success. In 1990 the first longitudinal clinical trial was published suggesting that implants could be loaded immediately or early in the mandibles of selected patients (Schnitman 1990). Nowadays immediate and early loaded implants are commonly used particularly in mandibles of good bone quality (Branemark 1999). Some authors also advocate that the use of some specific implant surface preparation is able to reduce the healing time (Rocuzzo 2001).

#### **2.5 Bioactive Calcium phosphate coating and S.L.A surface vitro comparison**

Alfa Gate "BioActive calcium phosphate (Cap) coated dental implants were tested at the Bruce Rapaport Faculty of Medicine at the Technion Institute of Technology to determine whether the TCP coating could induce Increased affinity, attachment and growth of bone forming cells (osteoprogenitors).

The study involved the culture of human osteoprogenitors on S.L.A surfaced and CaP coated Alfa Gate dental implants. Cell growth and metabolic activity were Followed in culture (10 Days) and the implants were examined by Scanning Electron Microscopy (SEM) to determine the presence of and adaptation of bone-forming cells on the TCP coated and standard implants, to test the stability of CaP coating

Bioactive CaP-coated implants demonstrated hydrophilic properties and human bone-forming cells attached readily to the surface interface while very few cells adhered to the S.L.A. surface.

Subsequent incubation on the implants, replication rates of osteoprogenitor cells was 600% greater on the CaP coated implant than on the S.L.A. surfaced implant.

SEM analysis revealed that bone-forming cells adhered to the entire surface area of the Bioactive implants. The cells demonstrated well formed projections and tissue-like monolayers.

#### **Materials and Methods**

Study of the 6 weeks function of 16 oral implants in 6 patients, in the mandibular clinical situations we have evaluated the clinical and para clinical parameters to predict implant outcomes and dynamic evolution .We initiated a short-term prospective study on Bioactive Alfa Gate implants. The following para clinical analyses were determined to access the necessary dates for success and survive rate of implants: The implant primary and changed stability of 6 weeks stability (the resonance frequency analysis (Osstell Mentor® (RFA) Osstell AB, Gothenburg, Sweden) which was done weekly and the result was registered to make the statistical comparison.

### 3.1 Inclusion criteria

The inclusion criteria were: patients eligible for enrolment were of either sex, older than 18 years of age who had received at least one Alfa Gate Bioactive implant (Alfa Gate) in the time period between January 2010 and February 2010; patient's agreement to a 6 weeks follow-up period; fixed prosthetic reha-bilitation. Exclusion criteria were: prosthetic treat-ment with removable prosthesis on implants, acute and chronic sinus infections, maxillary cysts, tumors, root tips, physical and psychiatric severe consider-ation that will affect the implant procedure or history of chemotherapy and radiotherapy of the maxillo-facial and cervical areas and severe smoking. There were, however, no restrictions on bone quality and quantity or addition bone grafting and regeneration procedures intended for implant placement. No other inclusion or exclusion criteria were applied.

### 3.2 Surgical Procedure

All surgeries were performed under local anaesthesia with 3 patient with open flap (fig. 3.1) and 3 with flapless (fig 3.2) access to the bone. Osteotomy preparations of neo alveolas were performed with low speed high-torque drill units using intense irrigation with a cold saline solution. During each site preparation of the neo alveolas for the implants, the bone quality II to III was recorded. All implants were placed manually and final torque was measured with a manual torque control wrench (fig 3.3) with result of 35-45 Ncm. And each implant was covered with healing abutment (fig 3.4) for easy access For the quantitative evaluation of implant stability, RFA was recorded with the Osstell Mentor device. Orthopan-tomographic X-ray images were used for calculation of radiological bone loss and the respective success criterion.

### 3.3 Measurement procedure.

Measurement procedure is done weekly with exact interval of 7 days, during this procedure the healing cap will be removed and

The smartpeg(fig 3.5) will be installed on the implant, Osstell will be used to measure the RFA from the transducer (fig 3.6).

After the result collection the smartpeg will be removed and a syringe with levomecol (fig 3.7) will be injected to the implant orifice, and the healing abutment will be installed again.

### 3.4 Statistics

For the statistical evaluation, implant-related data were calculated.

For statistical calculation, Fisher's exact test was used. A difference was considered to be significant when the p value was <0.05. The Kaplan-Meier survival function was used for the description of survival rates.

### Apertioation of reverce torque force for removing healing cap with out affecting implant stability

The aims of our proposed research are: determination the forces that is needed to insert the healing cap and the material that will act as enhancer for re-



Fig.3.1. open flap



Fig.3.2. flapless



Fig.3.3. torque wrench



Fig.3.4. Healing abutment



Fig.3.5. Smartpeg installed in the implant



**Fig. 3.6.** Osstell measurement



**Fig. 3.7.** levomecol injection

moving the healing cap with out any resistance torque or difficulties.

And to determine if the factor of time has any relation with healing cap implant resistance.

Our aims of the present study are: (1) Determination of the forces and material that needed to insert the healing cap (Alfa Gate) on the bioactive im-plant (Alfa Gate), without increasing resistance when removing the healing cap part, without affect-ing implant stability.

And to determine if the factor of time has any relation with increasing the healing cap implant connection resistance

We intend to perform a para-clinical research study to solve aims of our work.

By the results that we had measured during our test , not surprisingly the vasilin had the main lubrication effect during the reveres torque measurements.


But also we saw that the levomecol had a similar effect with a very minor differences, but on the other hand the levomecol have another antibacterial and anti-inflammatory effect, because it is Combined preparation containing chloramphenicol and Methyluracilum. So after this results of the test we recommend to use levomecol as lubrication material for the healing cap during the 6 weeks implants follow-up with Osstell and Alfa Gate implants.

### Documentation of implant stability dynamics during the 6 weeks.

#### 4.2.1 Stabily coefcient after insertion

**Table 4.2.1.1** Weekly data collection for the subjected implants.

Implant # / Week	0	1	2	3	4	5	6
1	59	80	73	71	70	70	70
2	66	52	68	75	73	70	70
3	62	62	53	62	68	69	70
4	62	55	59	62	64	64	65
5	76	70	75	89	81	82	83
6	69	66	68	73	75	74	74
7	67	60	66	70	71	71	71
8	61	65	66	67	68	69	69
9	76	64	68	68	68	68	68
10	78	78	80	74	73	73	73
11	82	76	78	74	72	72	72
12	73	72	70	65	67	67	68
13	58	51	59	64	68	72	72
14	65	62	63	66	67	67	68
15	64	60	61	65	68	70	70
16	64	61	63	67	67	69	69
MEAN	67.625	64.625	66.875	69.5	70	70.438	70.75

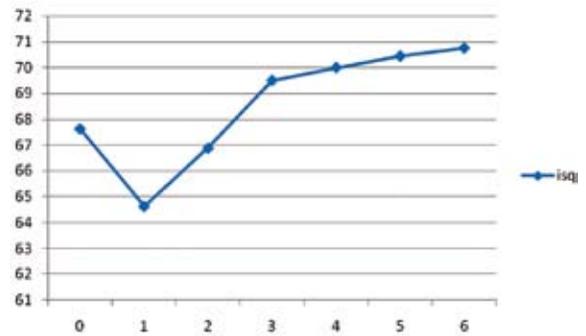

**Fig 4.2.1.8** Dynamic evolution of the measured implant during the 6 weeks, from week 0 which is at surgery time, we can notice the sharp reduction of Implant stability after one week from surgery with ISQ mean of 64.63, which is the losing of mechanical stability , and till the week 4 it is critical time for implant osseointegration, and in week 6 all implants has ISQ more than 65 which is the stability required for implant prosthetic

**Table 4.2.1.9** Measurement deviation

	N	Mini- mum	Maxi- mum	Mean	Std. Devia- tion
V18	7	64.63	70.750	68.23	2.29
Valid N (listwise)	7				

Measurement deviation of ISQ value during the 6 weeks research, the Standard deviation of 2.29 and the mean was 68.23 ,the maximum ISQ value was recorded was 70.75 ISQ at week six and the minimum ISQ value that was recorded is 64.63 ISQ at week 1 after surgery, as we notice after one wek implant loss the mechanical stability and at week 6 implant have a high biological stability, wich is recommended for implant loading.

In the data that was collected, we can notice that during the first and the second week the mean stability was reduced and from the third week started to

have increase in the mean stability coefficient., tell the week 6 we had a mean of 70.75 ISQ and the minimal was 65 ISQ, which by the recommendation of Other studies, for loading. This phenomena very noticeable in (figure 4.2.15), and in this specific week all the studied implant had an ISQ MORE THAN 65.

### 5. Conclusions:

1. The stability dynamics of Alfa Gate Bioactive implant showed, that during the first till fourth week it has the minimum implant stability with critical time in implant bone integration.
2. During the sixth week after implantation the stability coefficient for all implants was more than 65 ISQ, which was possible for implant loading.
3. The elaboration method in vivo that was used during this research is inoffensive and may be used in other studies.

### Literature:

1. Akca K, Chang TL, Tekdemir I, Fanuscu MI. Biomechanical aspects of initial intraosseous stability and implant design: a quantitative micro-morphometric analysis. *Clin Oral Implants Res.* 2006;17:465–472.
2. Albrektsson T, Wennerber A. (2004) Oral implant surfaces: part 2—review focusing on clinical knowledge of different surfaces. *International Journal of Prosthodontics* 17: 544–564.
3. Albrektsson T, Zarb G, Worthington P, Ericson RA. The long term efficacy of currently used dental implants: a review and proposed criteria of success. *Int J Oral Maxillofac Implants* 1986; 1:11.
4. Al-Nawas B, Groetz KA, Goetz H, Duschner H, Wagner W. Comparative histomorphometry and resonance frequency analysis of implants with moderately rough surfaces in a loaded animal model. *Clin Oral Implants Res.* 2008 Jan;19(1):1-8.
5. Al-Nawas B, Hangen U, Duschner H, Krummenauer F, Wagner W. Turned, machined versus double-etched dental implants in vivo. *Clin Implant Dent Relat Res.* 2007 Jun;9(2):71-8.
6. Alsaadi G, Quirynen M, Komarek A, van Steenberghe D. Impact of local and systemic factors on the incidence of late oral implant loss. *Clin Oral Implants Res.* 2008;19:670–676.
7. Aparicio, C., Rangert, B. Sennerby, L. Immediate/early loading of dental implants: a report from the Sociedad Espanola de Implantes World Congress consensus meeting in Barcelona, Spain, 2002. *Clinical Implant Dentistry and Related Research* 5: 57–60.
8. Balleri P, Ferrari M, Veltri M. One-Year Outcome of Implants Strategically Placed in the Retrocanine Bone Triangle. *Clin Implant Dent Relat Res.* 2009 Apr 23. [Epub ahead of print]
9. Behneke A, Behneke N. Recall and aftertreatment. In: Koeck B, Wagner W, eds. *Praxis der Zahnheilkunde*. München: Urban&Fischer, 2005:315–350.
10. Berdougou M, Fortin T, Blanchet E, Isidori M, Bosson JL. Flapless Implant Surgery Using an Image-Guided System. A 1- to 4-Year Retrospective Multicenter Comparative Clinical Study. *Clin Implant Dent Relat Res.* 2009 Feb 13. [Epub ahead of print]
11. Buser D, Brägger U, Lang NP, Nyman S. Regeneration and enlargement of jaw bone using guided tissue regeneration. *Clin Oral Implants Res* 1990; 1:22–32.
12. Chiapasco, M., Gatti, C. Implant-retained mandibular overdentures with immediate loading: a 3- to 8-year prospective study on 328 implants. *Clinical Implant Dentistry and Related Research* 5: 29–38.
13. Cochran D, Schenk R, Lussi A, Higginbottom F, Buser D. (1998) Bone response to unloaded and loaded titanium implants with a sandblasted and acid-etched surface: a histometric study in the canine mandible. *Journal of Biomedical Materials Research* 40: 1–11.
14. De Rouck T, Collys K, Cosyn J. Immediate single-tooth implants in the anterior maxilla: a 1-year case cohort study on hard and soft tissue response. *J Clin Periodontol* 2008; 35: 649–657

15. Fermbergård R, Astrand P. Osteotome sinus floor elevation and simultaneous placement of implants—a 1-year retrospective study with Astra Tech implants. *Clin Implant Dent Relat Res.* 2008 Mar;10(1):62-9.
16. Glauser R, Lundgren AK, Gottlow J, Sennerby L, Portmann M, Ruhstaller P, Hämmerle CH. Immediate occlusal loading of Brånemark TiUnite implants placed predominantly in soft bone: 1-year results of a prospective clinical study. *Clin Implant Dent Relat Res.* 2003;5 Suppl 1:47-56.
17. Glauser R, Sennerby L, Meredith N, Ree A, Lundgren, A., Gottlow J, Hammerle C.H. Resonance frequency analysis of implantssubjected to immediate or early functional occlusal loading. Successful vs. failing implants. *Clinical Oral Implants Research.* 2004. 15: 428–434.
18. Iqbal MK, Kim S. For teeth requiring endodontic treatment, what are the differences in outcomes of restored endodontically treated teeth compared to implant-supported restorations? *Int J Oral Maxillofac Implants* 2007; 22(Suppl):96– 116. (Review. Erratum in: *Int J Oral Maxillofac Implants* 2008;23(1):56).
19. Irinakis T, Wiebe C. Clinical evaluation of the NobelActive implant system: a case series of 107 consecutively placed implants and a review of the implant features. *J Oral Implantol.* 2009;35(6):283-8.
20. Jimenez D, Shah K, El-Ghareeb M, Aghaloo T, Pi-Anfruns J, Hameed S, Chiang J, Judge N, Ivry B, Wakimoto M, Moy P. Use of Osstell for determination of implant staging and loading protocols to improve implant success rates. Poster presentation AO, 2009.
21. Junker R, Dimakis A, Thoneick M, Jansen JA. Effects of implant surface coatings and composition on bone. *Clin. Oral Impl. Res.* 20 (Suppl. 4), 2009; 185–206.
22. Kahraman S, Bal BT, Asar NV, Turkyilmaz I, Tözüm TF. Clinical study on the insertion torque and wireless resonance frequency analysis in the assessment of torque capacity and stability of self-tapping dental implants. *J Oral Rehabil.* 2009 Oct;36(10):755-61.
23. Kullman L, Al-Asfour A, Zetterqvist L, Andersson L. Comparison of radiographic bone height assessments in panoramic and intraoral radiographs of implant patients. *Int J Oral Maxillofac Implants* 2007; 22:96–100.
24. Kullman L, Al-Asfour A, Zetterqvist L, Andersson L. Comparison of radiographic bone height assessments in panoramic and intraoral radiographs of implant patients. *Int J Oral Maxillofac Implants* 2007; 22:96–100.
25. Le Guehennec L, Goyenvalle E, Lopez-Heredia M.A, Weiss P, Amouriq, Y, Layrolle P. (2008) Histomorphometric analysis of the osseointegration of four different implant surfaces in the femoral epiphyses of rabbits. *Clinical Oral Implants Research* 19: 1103–1110.
26. Lekholm U, Zarb GA. Patient selection and preparation. In: Brånemark PI, Zarb GA, Albrektsson T, eds. Chicago: Quintessence Publishing Co., 1985:199–209.
27. Maló P, Friberg B, Polizzi G, Gualini F, Vighagen T, Rangert B. Immediate and early function of Brånemark System implants placed in the esthetic zone: a 1-year prospective clinical multicenter study. *Clin Implant Dent Relat Res.* 2003;5 Suppl 1:37-46.
28. Rabel A, Kohler SG, Schmidt-Westhausen AM. Clinical study on the primary stability of two dental implant systems with resonance frequency analysis. *Clin Oral Investig.* 2007;11:257–265.
29. Schwarz S, Gabbert O, Hassel AJ, Schmitter M, Séché C, Rammsberg P. Early loading of implants with fixed dental prostheses in edentulous mandibles: 4.5-year clinical results from a prospective study. *Clin Oral Implants Res.* 2010 Jan 13. [Epub ahead of print].
30. Tarnow, D.P., Emtiaz, S., Classi, A. Immediate loading of threaded implants at stage I surgery in edentulous arches: ten consecutive case reports with 1- to 5-year data. *International Journal of Oral and Maxillofacial Implants* 12: 319–324.
31. Topalo V., Dobrovolschi O. Metodă miniinvazivă de instalare a implantelor dentare endosoase. *Buletinul Academiei de Ştiinţi al R. Moldova* 2008.
32. Valentin Topalo, d.h.m., Oleg Dobrovolschi, Resorbţia osului cortical periimplantar în perioada osteointegrării implantelor dentare endosoase. *Revista medicina stomatologică*, 2009, nr. 4(13), p. 41-46.